



# Micro OWL Optical Power Meter

Operations Manual  
Firmware Version 1.18e  
November 26, 2002  
OWL Part# MO-1xx

## Table of Contents

Preface	ii
Unit 1 - Introduction	
Description	1-1
Applications	1-1
General Features	1-2
Keyboard Entry Method	1-2
Unit 2 - Meter Functions	
Operation	
Power ON	2-1
Power Units Supported by the Micro OWL	2-1
Wavelengths Supported by the Micro OWL	2-2
"Zeroing" the Micro OWL	2-2
Monitor Mode	2-2
Main Menu	2-3
Meter Setup	2-3
Manual Reference Method	2-4
Stored Data Menu	2-4
Power OFF	2-5
Unit 3 - Fiber Certification	
Overview	3-1
Operation	3-1
Power ON	3-1
Fiber Certification	3-1
Definition of a Link	3-1
Required Equipment	3-1
Preparation	3-1
Reference Method	3-1
Step 1 - Select Link	3-2
Step 2 - Define Link	3-2
Step 3 - Take Readings	3-3
Step 4 - Stored Data	3-3
UNIT 4 - Appendices	
Appendix A - Decibel Review	4-1
Appendix B - Dynamic Range Review	4-2
Appendix C - Glossary	4-2
Appendix D - Micro OWL Specifications	4-6
Appendix E - Warranty Information	4-6
Appendix F - Cleaning and Care Instructions	4-7
Appendix G - Supplies	4-8
Appendix H - Link Budget Calculation Worksheet	4-9
Appendix I - Reference Jumper Setup	4-10

## Why Use An Optical Fiber Power Meter?

Standards organizations such as the TIA or the ISO/IEC provide performance standards that the cabling plant must adhere to in order to support high-speed protocols such as Gigabit Ethernet. Fiber can be tested against these standards, ensuring that it is able to handle the high amount of traffic with a maximum amount of reliability.

These standards organizations also provide standards for administration of the cabling plant. These standards require a fiber link to be certified; that is, a report must be generated from appropriate test equipment for tracking and auditing purposes. These reports can also be used as verification of compliance to performance standards in case a question comes up about the quality of an installation. These signed documents cover the installer from liability provided that the link meets specified performance standards.

Our optical fiber power meters are designed with these standards in mind because we understand the importance of qualifying your fiber installations with standards-compliant test equipment. The meter you have just purchased also prints professionally formatted reports showing the conformity to these popular industry standards. You can print out these reports as a record of the original conformity to quality set by the standards. These documents signed by all associated parties may prove valuable in any future disputes concerning the installation.

## Checking The Micro OWL Firmware Version

This manual is written for the Micro OWL firmware version 1.18e. It is not valid for previously released Micro OWL versions. Follow the instructions below to verify the meter's firmware version.

- 1) Press **ON** to start up the meter.
- 2) After the owl flies across the initial boot-up screen, the display should look like the diagram below. This screen only remains viewable for approximately 2 seconds.

If the firmware version is not V1.18e, check our website at [OWL-INC.COM](http://OWL-INC.COM) for the correct version of the manual.

Company Name  
Company Phone  
Serial Number  
Firmware Version

```
.....  
.....  
SN: MOXXXXX  
V1.19e
```

## Description

The Micro OWL is a high accuracy, high resolution, microprocessor controlled, optical power meter. The meter has a wide dynamic range making it ideal for both single and multi-mode fiber testing.

It has an attractive handheld case, a backlit graphical liquid crystal display, and 18-key keypad for easy data entry. The meter comes with a small state-of-the-art UNIVERSAL adapter that is fully reliable for the use of ST, SC, FC or any 2.5 mm connectors which saves *money on consumables* (test cables wear out). It will operate for over 100 hrs on a single 9v battery and has built in auto shutdown.

The Micro OWL includes a built-in link wizard that helps the user easily calculate the allowable loss for the fiber runs that they will be measuring. The meter stores physical fiber information for up to four links. Link information includes: link name, date, fiber type, fiber length, connectors, splices, temperature, and calculated or entered reference power values for four wavelengths. In addition the meter will store up to 1000 measured data points with labels. Each value includes the fiber type and link.

The stored information can be selectively viewed, edited (measured again), printed, or deleted. The meter will print formatted reports of selected stored data directly using the built in serial port, or all of the stored data can be downloaded to a computer spreadsheet or our free OWL Reporter software to produce professional-looking formatted certification reports.

## Applications

The Micro OWL can be used for several applications. A listing of these applications and their descriptions follows:

**Attenuation and Loss Measurements** - After a fiber cable has been installed and terminated, it must be tested to determine if the fiber is installed correctly. A comparison of the actual power measurement and the reference value determines the loss of the fiber link.

**Fiber Network Certification** - The Micro OWL uses a loss wizard that is used for fiber certification against the popular industry cabling standard called the EIA/TIA 568-A. The user is prompted to enter several parameters, which allows the Micro OWL to calculate a certification reference value and store it in the meter. As the user stores data points in the meter using the loss wizard, the actual power level of the link is also stored. The data is then downloaded into our OWL Reporter software, where the actual power value is compared to the reference value. Certification reports can be printed out with details or summaries of the fibers being certified.

**Fiber Continuity Testing** - Continuity can be measured with the Micro OWL by placing a calibrated light source on one end of the fiber and the Micro OWL on the other end. This is also a simple way to measure the attenuation of the fiber.

**Patch Cord Testing** - Fiber links that are producing incorrect results may have bad patch cords. The Micro OWL can be used to test the attenuation of a patch cord to see if it is usable, or should be thrown out.

**Active Equipment Optical Power Measurements** - Active equipment needs to be measured periodically for correct power levels and stability. The transmitters in this equipment have a known power value. The Micro OWL can be directly attached to this equipment via a patch cord to check whether the transmitter is stable and is within the manufacturer's specified power range.

## General Features

- 1 **2.5mm UNIVERSAL ADAPTER PORT** - accepts standard 2.5mm ferrule connectors (ST, SC, FC).
- 2 **COMPUTER PORT** - port for downloading data from the meter to a PC via serial cable.
- 3 **LIQUID CRYSTAL DISPLAY (LCD)** - displays power readings, menus, and information necessary for operation of the meter. The elements of the display are discussed in the appropriate units.
- 4 **FUNCTION KEYS** - activate the options on the Function Options Menu.
- 5 **ALPHA NUMERIC KEYS** - enter letters, numbers, and symbols into field prompts.
- 6 **MENU KEY** - used to enter the menu system.
- 7 **DONE KEY** - activates certain menu options.
- 8 **BACK LIGHT KEY** - toggles the LCD back light ON or OFF.
- 9 **ON/OFF KEYS** - turns the meter ON or OFF.

If your Micro OWL has the optional LED light source installed, the **4** key is used to turn it on and off.



## Keyboard Entry Method

Several screens in the Micro OWL menu system require the user to enter some input, e.g. a fiber length measurement or a descriptive name for a fiber run. This feature allows the Micro OWL to become more user-friendly.

**ALPHA-NUMERIC FIELDS.** These fields allow the user to enter either a number, a letter, or a special character. This is accomplished by pressing and holding the key until the desired character appears. When the key is released, the cursor automatically advances to the next position.


**NUMERIC FIELDS.** These fields are for numeric input only, e.g. fiber length, user-defined reference values, etc. The cursor will automatically advance once a number key is pressed. **EXCEPTION:** some numeric operators may be required, such as the minus sign, or a decimal point. Special characters reside under the **0** key. In this case, they are treated like alpha-numeric fields.

Press the **DONE** key when character input is complete.

## Operation

### Power On

- 1) Press the **ON** button.
- 2) After a few seconds, a screen will appear that looks like the one below, which is called Immediate Mode.

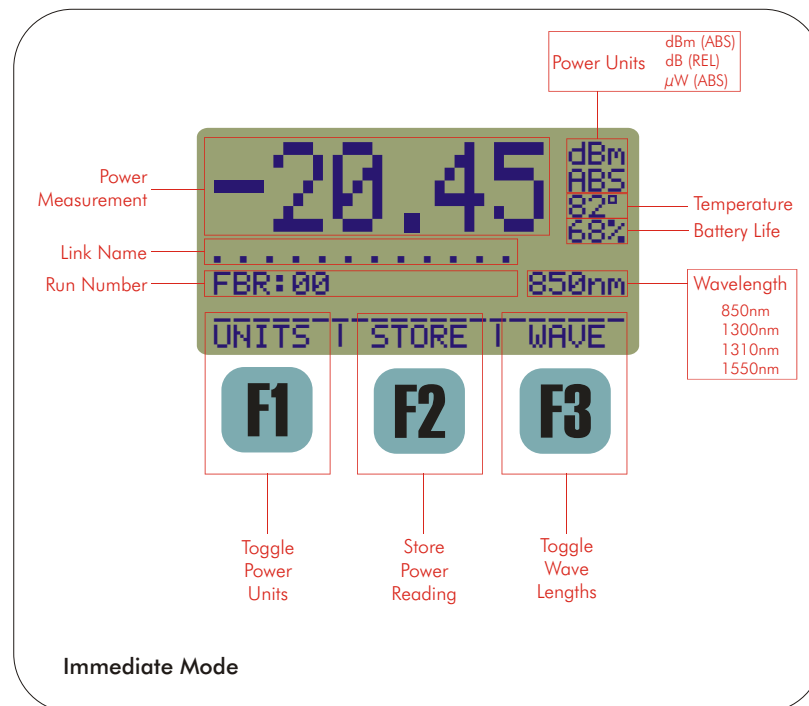

### Power Units

The Micro OWL is capable of displaying power readings in three different units. The user may toggle through these units by pressing **F1**:

**dBm (ABS)** - This is an absolute (ABS) power measurement. It shows how much optical power is being received by the photodetector in decibels referenced to a milliwatt (dBm).

**dB (REL)** - This is a relative (REL) power measurement. It shows the amount of optical power being received by the photodetector relative to a user-defined reference power (i.e. "zeroing" the meter). If a reference value has been set, toggling to REL mode will show the user how much optical power is being lost in the link.

**μW (ABS)** - This is an absolute (ABS) power measurement. It shows the amount of optical power being received by the photodetector in microwatts, or millionths of a watt.

## Operation, cont.

### Wavelengths

Measurements can be taken for four different wavelengths in the Micro OWL. These wavelengths are 850, 1300/1310, and 1550nm. All wavelengths are traceable to the National Institute of Standards and Technology (NIST). The user may toggle through these wavelengths by pressing **F3**.

### “Zeroing” the Micro OWL in Immediate Meter mode

This function allows the user to set references for each wavelength for fiber attenuation testing.

After connecting a light source to the Micro OWL:

1. Toggle the wavelength until it matches the wavelength of the source.
2. Press **0** to zero the meter. The user will be prompted to verify the set reference.
3. Press either **F1** to set the reference, or **F3** to abort.

**NOTE: When using laser sources, allow the laser to warm up according to the manufacturer specifications to ensure accurate references.**

**NOTE: When zeroing multiple wavelengths, do NOT remove the patch cord from the light source. Removing the patch cord from the light source will invalidate the optical reference for the wavelength that was just set. Use a separate patch cord for each light source port.**



### Monitor Mode

Monitor Mode sends absolute power measurements in a comma delimited format to the serial port in real time. A terminal program is required to view data in real time.

To enter Monitor Mode, press **5**, and press **DONE** to return to Immediate Mode.



### Integrated Light Source (optional)

If your Micro OWL has an integrated light source, press **5** to turn it ON and OFF.


To enter Monitor Mode, press **5**, and press **DONE** to return to Immediate Mode.



## Operation, cont.

### Main Menu

Advanced meter functions can be configured from the Main Menu. Options 1 through 4 are listed in a step-by-step order for certifying fiber links and will be explained in greater detail later in this manual. Option 5 is explained below. Press **MENU** to enter the MAIN MENU.

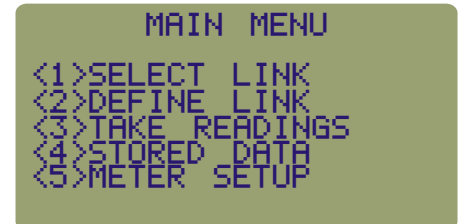

**SELECT LINK** **1** **ABC** This option allows the user to select the fiber link to be used for the test, as well as editing its descriptive name and test date.

**DEFINE LINK** **2** **DEF** This option is used to define the parameters of the fiber link which are used to calculate the link's PASS/FAIL threshold.

**TAKE READINGS** **3** **DEF** This option takes the user to the main display screen, where they can view power readings, store data points, and switch wavelengths.

**STORED DATA** **4** **DEF** This option allows the user to view and download the data points previously stored in the meter.

**METER SETUP** **5** **DEF** This option allows the user to edit the owner information, and adjust the LCD contrast.

Pressing **DONE** from the MAIN MENU will return the user to the power reading display screen.

### Meter Setup

From the MAIN MENU, press **5** to enter the METER SETUP menu. From this menu the user can change company information, such as name and phone number, and can also adjust the contrast of the LCD screen.

**F1** – changes the company name. Edit the company name and press **DONE** to continue.

**F2** – change the company telephone number. Edit the company telephone number and press **DONE** to continue.

**F3** – adjust the contrast of the LCD display. Press **F1** or **F3** to set the contrast down or up. Press **DONE** to continue.



## Operation, cont.

### Manual Reference Method-**recommended for advanced users only**

The Micro OWL can be used to certify fiber links (shown in detail in the next unit) or to measure link loss by setting a manual reference. The manual reference method is used to measure the actual loss in a fiber link, and it is recommended that only those users who are very familiar with calculating link budgets should use this method.

- 1) From Immediate Mode, press **MENU** to enter the MAIN MENU.
- 2) At the MAIN MENU, press **1 ABC** to SELECT LINK. Highlight a link, and press **F3** to change the name and/or date. Press **DONE** to continue.
- 3) Press **F2** to LOAD the selected link, and press **DONE** to continue.
- 4) From the MAIN MENU, press **2 DEF** to DEFINE LINK. Press **2 DEF** to SET A MANUAL REFERENCE. **NOTE: setting a reference with this method will overwrite any previous certification or manual references.**
- 5) Press **F1** to scroll through the wavelengths, and press **F2** to set the manual reference. The asterisk shows the currently selected wavelength.
- 6) Type in the manual reference using the keypad, and press **DONE** to continue. Press **DONE** to return to the MAIN MENU.
- 7) Press **3 GHI** to return to Immediate Mode and TAKE READINGS. Data storage is covered in more detail in the next unit.

## Stored Data Menu

The STORED DATA menu allows the user to manipulate data that is stored in the Micro OWL.

**VIEW/EDIT/LOAD 1 ABC** - this option allows the user to view, edit, or load any data point that was previously stored in the Micro OWL. The VIEW/EDIT/LOAD screen initially loads with the first data point stored in memory. To go to a different data point, use: **F1** to scroll through the fiber names; **F2** to scroll through the fiber runs for the currently selected fiber name; or **F3** to scroll through the wavelengths for the currently selected data point.

Pressing **0** will LOAD the selected data point, and return the user to Immediate Mode showing the selected data point. From there, the user can continue saving data from that point.

Pressing **5 MENU** will EDIT (or reshoot) the selected data point. The user will be returned to Immediate Mode to re-save the data point. After the data point is re-saved, the user is returned to the last data point that was previously stored.

**PRINT RANGE 2 DEF** - this option allows the user to print data points to a serial device, such as a serial printer or terminal program. The printout is formatted in an easy-to-read format.

**DELETE RANGE 3 GHI** - this option allows the user to delete a range of data points, or delete all of the data points from the meter. This should only be done after the data points have been downloaded into the PC with OWL Reporter software.

**DOWNLOAD DATA 4 JKL** - this option allows the user to download data either to OWL Reporter software, or to a terminal program. Data downloaded to a terminal program is in a Comma-Delimited format for easy placement into a program that can format Comma-Delimited files. The PC must be connected to the meter via the Micro OWL download cable.

## Operation, cont.

If the user is downloading to OWL Reporter, then no further action is necessary from this screen. OWL Reporter will handle the data transfer.

If the user is downloading to a terminal program, then the user must start the terminal program, and press **F1** to begin the download.

## Power OFF

Press **OFF** to shut down the Micro OWL. The user will be prompted to verify shutdown.

## Overview

The whole purpose of fiber certification with the Micro OWL is to save data points using a standards-based reference point and produce professional-looking reports for the customer.

The Micro OWL is capable of storing up to 1000 data points with user-configurable fiber labels, and can certify up to four separate fiber links against the EIA/TIA 568-A standard.

Data points are downloaded into our free OWL Reporter Windows-compatible software for organizing data points and printing professional-looking certification reports.

## Operation


### Power On

Press the **ON** button. After a few seconds, the meter will display Immediate Mode (see Unit 2 for a description of the screen).

### Fiber Certification

Before we begin, it is important to understand the term 'LINK' as it is used in the Micro OWL.

*Definition of a link:* In the Micro OWL, a link is defined as any number of fibers, or fiber runs, that all have the same set of fiber characteristics from one end to the other; typically begin together and end together; and follow the same pathway. These characteristics include fiber length, fiber type, connector loss, and splice loss, and the cabling standard being used for fiber certification. **NOTE: Any time one of these fiber characteristics changes, a new link must be configured.**

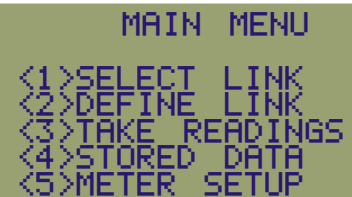

```
MAIN MENU
<1>SELECT LINK
<2>DEFINE LINK
<3>TAKE READINGS
<4>STORED DATA
<5>METER SETUP
```

## REQUIRED EQUIPMENT

To perform fiber certification with the Micro OWL, the user will need the following equipment:

- Micro OWL optical power meter
- Stabilized light source (multi-mode or single mode, depending upon fiber type being tested)
- Power meter test jumper (make sure the connectors match the fiber under test)
- Light source test jumper (the user will need one jumper for each connector port on the light source)
- Mandrel (1/2 inch; only for multi-mode fiber certification; the user will need one mandrel for each light source jumper)

## PREPARATION

Make sure all of the required equipment is working properly:

- Clean the connector ports on the meter and light source (see Appendix F for cleaning instructions)
- Allow the light source to warm up according to manufacturer recommendations
- Clean and test the jumpers to make sure they are not adding significant loss to the test

## REFERENCE METHOD - (see Appendix I for more details)

For proper certification of fiber links using the Micro OWL, use the following methods for setting certification references:

- Single mode fiber - EIA/TIA 526-7, Method 1.A
- Multi-mode fiber - EIA/TIA 526-14A, Method B

The following steps (Options 1 through 4 on the MAIN MENU) outline the procedure for setting up the Micro OWL for fiber certification. The MAIN MENU takes the user through a step-by-step process to certify fiber links. This step-by-step process is called the Link Wizard.

The Link Wizard calculates a PASS/FAIL threshold according to the link attenuation values detailed in the TIA/EIA 568-A cabling standard. All fibers included in the link are measured against this threshold to produce a PASS or FAIL reading.

*Fiber Certification, cont.*

## STEP 1 - SELECT LINK

1-1) Press **MENU** to enter the MAIN MENU.

1-2) Press **1** to SELECT LINK.

1-3) At the STORED LINKS menu, the currently loaded link is denoted by an asterisk. Scroll through the list of links by pressing **F1** to highlight the link to use. Press **F3** to edit the name and the testing date of the selected link.

### EDIT LINK

1-3a) Give the link a descriptive name. Press **F1** to edit the name. Press **DONE** to continue.

1-3b) Enter the date of the test. Press **F2** to enter the date. Press **DONE** to continue.

1-3c) When the name and date have been entered, press **DONE** to return to the STORED LINKS menu.

1-4) Press **F2** to load the selected link. The user will be returned to the MAIN MENU.

## STEP 2 - DEFINE LINK

2-1) Press **2** to DEFINE LINK.

2-2) Press **1** to CERTIFY LINK.

2-3) Scroll through the list of fiber types and highlight the link's fiber type. Press **F2** to select.

2-4) Enter the length of the fiber in meters. Press **DONE** to continue.

2-5) Enter the number of inline connections (connector pairs) in the link. Press **DONE** to continue.

2-6) Enter the number of inline splices in the link. Press **DONE** to continue.

2-7) Connect the light source for the wavelength shown on the display (remember: if the user is testing multi-mode fibers, the test jumper must be wrapped 5-7 times around a mandrel). Press **F1** or **DONE** to continue.

2-8) The settings the user just entered will appear on the display (see the example below).

**SRC PWR** (shown in dBm) - actual power the light source is emitting.

**100 m** (shown in dB) - attenuation value associated with the length and type of fiber the user entered.

**0 CONN** (shown in dB) - attenuation value of the connectors and splices the user entered.

**REF PWR** (dBm) - source power plus fiber attenuation plus connector and splice attenuation. This is the PASS / FAIL threshold.

**850nm** - wavelength that the reference is being set for.

**M6** - fiber type that the reference is being set for (M6 = 62.5μm multi-mode, M5 = 50μm multi-mode, SI = single mode indoor, SO = single mode outdoor).

2-9) If any of the fiber characteristics were entered incorrectly, press **F2**. The user will be asked to repeat steps 2-3 through 2-7.

2-10) Press **F3** to save the reference. NOTE: The reference will not be saved if the users does not press **F3**.

2-11) If the user is testing at an additional wavelength, press **F1**. The user will be prompted to connect a light source for the other wavelength as in step 2-7. Repeat steps 2-7 through 2-10 for all wavelengths the user is setting a reference for.

```

SRC PWR = -20.24
100 m   = -00.38
0 CONN  = +00.00
REF PWR = -20.62
850nm M6

-----
WAVE | EDIT | SAVE
LEN  | LINK | REF.
    
```

## Fiber Certification, cont.

2-12) Press **DONE** to continue. The user will be returned to the MAIN MENU.

### STEP 3 - TAKE READINGS

3-1) Press **3** to TAKE READINGS. The screen shown on the right will appear. Take a moment to familiarize yourself with this screen.

**F1** - toggles power units between dBm (ABS), dB (REL), and  $\mu$ m (ABS). In dB (REL) mode, the power measurement changes to show the power level relative to the Link Wizard reference, and tells the user if the link passes or fails according to the EIA/TIA 568 cabling standard. A power reading with a minus sign means that the link has failed the standard, and a plus sign means that the link passes.

**F2** - stores the data point in memory for later download and report printing. Each data point is conveniently stored with a user-definable name and an auto-numbering system. In the diagram on the right, the label is the 'FBR:' in the Fiber ID field. The '00' following the label is the auto-incrementing number. Each time a data point is stored for a specific wavelength, this number goes up by 1.

**F3** - toggles wavelength between 850nm, 1300nm, 1310nm, and 1550nm.

3-2) Press **F2** to STORE a data point. The user may be prompted to enter a label. The user does not have to change this label, but it is recommended to set the label to better describe the fiber runs being stored. Press **DONE** to continue.

3-3) The user will be prompted to enter the fiber type. This fiber type must match the fiber type chosen in the Link Wizard. Scroll through the fiber types with the **F1** key, and press **F2** to select. The user will only have to enter the fiber type if they have not saved a data point for the current label.

3-4) Press **F3** to save the current data point and continue on to the next fiber.

3-5) Repeat steps 3-2 and 3-4 for each data point to save. If the fiber label needs to be changed, press **F2** at the Data Point Save Screen and repeat steps 3-2 through 3-4.

3-6) If the user is testing at additional wavelengths, press **F3** to toggle to the next wavelength. The auto-increment number will begin at '00' again, and have the same label. Repeat steps 3-2 and 3-4 for each data point being saved.

### STEP 4 - STORED DATA


Before downloading certification data points to a PC, the user must first have installed free OWL Reporter software on it. The software may be downloaded from [http://owl-inc.com/literature/sub/htm/owl\\_reporter.htm](http://owl-inc.com/literature/sub/htm/owl_reporter.htm).

4-1) Press **MENU** to enter the MAIN MENU.


4-2) Press **4** to enter STORED DATA.

4-3) Press **4** to DOWNLOAD DATA.

4-4) Connect the Micro OWL to the PC via the download cable supplied with the meter.

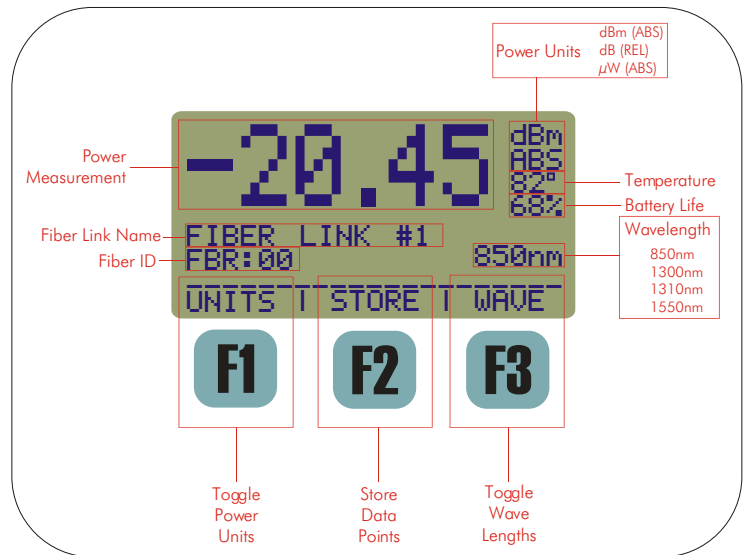

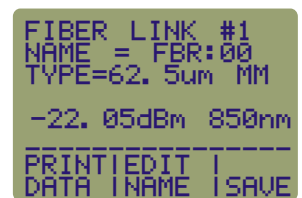

### dB (REL) Mode PASS/FAIL



### Data Point Save Screen

## *Fiber Certification, cont.*

4-5) Start the OWL Reporter software on the PC.

4-6) Click the Download option on the menu bar, or the Download button on the button bar. The data points that are stored in the meter will appear in the OWL Reporter window. Press  to return to the STORED DATA menu, and press  again to return to the MAIN MENU.

Once the data is downloaded into OWL Reporter, we recommend that the user saves them as an OWL Reporter file for permanent storage.

If hard copy of the data points is needed, the data points may be printed. There are two report options: summary and detail. The summary printout lists all of the data points together, shows whether the link passed or failed, and shows the power level of the fiber.

The detail printout prints each individual fiber run on a single page, and shows detailed information about the run, including whether the fiber passed or failed, and the remaining overhead of the fiber run.

## Appendix A - Decibel Review

The Micro OWL meter has a decibel(dB) range that spans 75dB. The whole purpose of your meter is to measure light energy in decibels. But what exactly is a decibel? It is not uncommon for a technician to be using an optical power meter and not understand what a decibel really is. If you struggle a little with this review, you will find the concept not so threatening.

This is what happens when we test a link: we send light of a specified wavelength from a stable light source down the fiber optic cabling. The meter then captures this light and measures it. As light travels down this path, however, its photons encounter impurities, connector gaps, and even the glass atoms themselves. All of these factors cause attenuation in the fiber. If there is too much attenuation, your fiber optic link will fail, because it does not have enough power to trigger the circuitry in the active receiver equipment. No communications can occur in this scenario.

Simply put, a decibel is a measure of the ratio of the power received at the end of a link relative to the power you started with, which is known. This fraction calculates the relative power. This calculation is similar to test scores or percentages.

$$\frac{\text{Amount of optical power left over at the end of the link}}{\text{Amount of optical power at the beginning of the link}} \times 100 = \text{Relative power out as a \%}$$

If test results were kept in percent or fractions, the average person wouldn't have difficulty in grasping the concept of decibels. Unfortunately, in scientific measurement, graphing power measurements has become too cumbersome due to their wide range of possible values; a person would need to paste lots of sheets of graph paper together to plot these power functions by hand. So scientists came up with a little trick to "squeeze" the graph down to a more presentable size. The trick uses logarithms (logs). Logs are fairly simple -- most of us have already encountered logs in pre-algebra class. They didn't seem so important then, but they are important to the understanding of decibels. Logs expressed in Base 10 are just a way to state how many zeros there are in a number.

For example,  $\log(10)=1$ ,  $\log(100)=2$ ,  $\log(1000)=3$ . Notice the pattern. Logs simply express how many places there are after the first number. Let's work with a number that isn't 10, 100, or 1000. For instance the  $\log(2014)=3.304$ . Notice that 2014 has three digits beyond the first, thus the "3" in the 3.304. Also notice how it relates to the "3" in  $\log(1000)=3$ . Remember, logs are a tool we use to "squeeze" our measurements down so they will fit on graph paper.

$$\text{LOG}\left(\frac{\text{Amount of optical power left over at the end of the link}}{\text{Amount of optical power at the beginning of the link}}\right) = \text{RELATIVE POWER AS A POWER OF 10}$$

Power is measured in Watts (W), therefore:

$$\text{LOG}\left(\frac{W_{\text{END OF LINK}}}{W_{\text{BEGINNING OF LINK}}}\right) = \text{RELATIVE POWER AS A POWER OF 10}$$

Mathematicians and scientists must have noticed that the shrinking effect of the graph was a little excessive. Logs in optical decibels get multiplied by 10. Thus we finally have:

$$10 \text{ LOG}\left(\frac{W_{\text{END OF LINK}}}{W_{\text{BEGINNING OF LINK}}}\right) = \text{RELATIVE POWER IN dB}$$

Remember: Decibels are simply the ratio of the power received by the receiver over the power sent out by the light source at the start of link.

### Appendix A - Decibel Review, cont.

There are other decibels to consider. The decibel we previously described is "dB" is called relative. This is because it is a ratio as was explained. With ratios there is no way to tell what absolute value we had at the start or end of a link. To solve the problem we can always reference our optical power to a fixed value of one milliwatt (1 mW). One milliwatt of power will replace the denominator of our equation.

$$10 \text{ LOG} \left( \frac{W_{\text{END OF LINK}}}{1 \text{ mW}} \right) = \text{ABSOLUTE POWER IN dB}$$

So when we are given a value of absolute power in dBm we know that it is the power relative to 1 mW and we can calculate the actual power in mW if necessary. We can also compare values in dBm to each other because they are relative to the same reference (1mW). However, we cannot compare values in dB to each other because we do not know if they are relative to the same reference.

### Appendix B - Dynamic Range Review

Now that you have a clearer understanding of the decibel, we can begin to study the dynamic range feature of the Micro OWL. The dynamic range of the Micro OWL is +5 to -70 dBm (or +25 to -70 dBm, but what exactly does this mean?

Dynamic range is defined as the difference between the minimum and maximum power levels that a photodetector can reliably sense, and still maintain acceptable accuracy. In the case of the Micro OWL, the dynamic range is 75dB.

Any power level reaching the detector that is greater than +5 dBm is too powerful to accurately measure. Likewise, any power level below -70 dBm will be too weak to be sensed.

Power levels within the dynamic range produce acceptable readings. It is interesting to note that the Micro OWL remains accurate over the upper 96% of the 75 dB dynamic range and then gets progressively worse as the power levels drop off.

The limits of dynamic ranges depend on certain factors. The minimum level depends on the sensitivity of the receiver. The sensitivity of the receiver can be increased by using different materials, such as germanium (Ge) or indium/gallium/arsenide (InGaAs). The characteristics of these materials allows the detector to be responsive at lower power levels. The maximum level depends on both the size of the receiver area, and also the amplifier used.

### Appendix C - Glossary

*Absorption.* The loss of power in an optical fiber, resulting from conversion of optical power into heat and caused principally by impurities, such as transition metals and hydroxyl ions, and also by exposure to nuclear radiation.

*Acceptance Angle.* The half-angle of the cone within which incident light is totally internally reflected by the fiber core. It is equal to  $\arcsin(\text{NA})$ .

*Attenuation.* A general term indicating a decrease in power from one point to another. In optical fibers, it is measured in decibels per kilometer at a specified wavelength.



## Appendix C - Glossary, cont.

*Bandwidth.* The transmission capacity of a system.

*Buffering.* 1. A protective material extruded directly on the fiber coating to protect the fiber from the environment (tight buffering). 2. Extruding a tube around the coated fiber to allow isolation of the fiber from stresses on the cable (loose buffered)

*Buffer Tubes.* Loose-fitting covering over optical fibers used for protection and isolation.

*Bundle.* Many individual fibers contained within a single jacket or buffer tube. Also, a group of buffered fibers distinguished in some fashion from another group in the same cable core.

*Cladding.* The outer concentric layer that surrounds the fiber core and has a lower index of refraction.

*Connector.* A mechanical device used to provide a means for aligning, attaching, and achieving continuity between fibers.

*Consolidation Point.* A location for interconnection between horizontal cables that extend from building pathways and horizontal cables that extend into work area pathways.

*Core.* The central, light-carrying part of an optical fiber; it has an index of refraction higher than that of the surrounding cladding.

*Cross-Connection.* A connection scheme between cabling runs, subsystems, and equipment using patch cords or jumpers that attach to connecting hardware on each end.

*Decibel (dB).* In fiber optics, a standard logarithmic unit for the ratio of the power that was received over the power that was originally sent.

*dBm.* Decibel referenced to a milliwatt.

*dBμ.* Decibel referenced to a microwatt.

*Detector.* An optoelectronic transducer used in fiber optics for converting optical power to electric current. In fiber optics, usually a photodiode.

*Diffraction.* The bending of radio, sound, or light waves around an object, barrier, or aperture edge.

*Dispersion.* A general term for those phenomena that cause a broadening or spreading of light as it propagates through and optical fiber. the three types are modal, material, and waveguide.

*Entrance Facility.* An entrance to a building for both public and private network service cables including the entrance point at the building wall and continuing to the entrance room or space.

*Equilibrium Mode Distribution (EMD).* The steady modal state of a multimode fiber in which the relative power distribution among modes is independent of fiber length.

### Appendix C - Glossary, cont.

*Equipment Room.* A centralized space for telecommunications equipment that serves the occupants of the building. Equipment housed herein is considered distinct from a telecommunications closet because of its nature or complexity of the equipment.

*Frequency.* Of a periodic wave, the number of identical cycles per second. Usually expressed in Hertz.

*Fresnel Reflection.* The reflection that occurs at the planar junction of two materials having different refractive indices; Fresnel reflection is not a function of the angle of incidence.

*Graded-index Fiber.* An optical fiber whose core has a nonuniform index of refraction. The core is composed of concentric rings of glass whose refractive indices decrease from the center axis. The purpose is to reduce modal dispersion and thereby increase fiber bandwidth.

*Horizontal Cross-Connect (HC).* A cross-connect of horizontal cabling to other cabling, e.g., horizontal, backbone, equipment.

*Index of Refraction.* The ration of the velocity of light in free space to the velocity of light in a given material.

*Insertion Loss.* The loss of power that results from inserting a component, such as a connector or splice, into a previously continuous path.

*Interconnection.* A connection scheme that provides for the direct connection of a cable to another cable or to an equipment cable without a patch cord or jumper.

*Intermediate Cross-Connect (IC).* A cross-connect between the main cross-connect and the horizontal cross-connect in backbone cabling.

*Laser.* Light Amplification by Stimulated Emission of Radiation. A light source producing, through stimulated emission, coherent, near monochromatic light. Lasers in fiber optics are usually solid-state semiconductor types.

*Light-Emitting Diode (LED).* A semiconductor diode that spontaneously emits light from the PN junction when forward current is applied.

*Main Cross-Connect (MC).* The cross-connect in the main equipment room for connecting entrance cables, backbone cables, and equipment cables.

*Material Dispersion.* Dispersion resulting from the different velocities of each wavelength in an optical fiber.

*Modal Dispersion.* Dispersion resulting from the different transit lengths of different propagating modes in a multimode optical fiber.

*Mode.* A possible path followed by light rays.

**Appendix C - Glossary, cont.**

*Multi-mode Fiber.* A type of optical fiber that supports more than one propagating mode.

*Numeric Aperture (NA).* The number that expresses the light-gathering ability of a fiber.

*Optical Time Domain Reflectometry (OTDR).* A method of evaluating optical fibers based on detecting backscattered (reflected) light. Used to measure fiber attenuation, evaluate splice and connector joints, and locate faults. Also, the equipment used to perform such measurements (Optical Time Domain Reflectometer).

*Photodetector.* An optoelectronic transducer, such as a PIN photodiode or avalanche photodiode.

*Photodiode.* A semiconductor diode that produces current in response to incident optical power and used as a detector in fiber optics.

*Photon.* A quantum of electromagnetic energy; a particle of light.

*Receiver.* An electronic device which converts optical signals to electrical signals.

*Responsivity.* The ratio of a photodetector's electrical output to its optical input in an optical fiber.

*Single Mode Fiber.* An optical fiber that supports only one mode of light propagation above the cutoff wavelength.

*Source.* The light emitter, either an LED or laser diode, in a fiber optic link.

*Spectral Width.* A measure of the extent of a spectrum. For a source, the width of wavelengths contained in the output at one half of the wavelength of peak power. Typical spectral widths are 20 to 60 nm for an LED and 2 to 5 nm for a laser diode.

*Splice.* An interconnection method for joining the ends of two optical fibers in a permanent or semi-permanent fashion.

*Step-Index Fiber.* An optical fiber, either multi-mode or single mode, in which the core refractive index is uniform throughout so that a sharp step in refractive index occurs at the core-to-cladding interface. It usually refers to a multi-mode fiber.

*Telecommunications Closet (TC).* An enclosed space for housing telecommunications equipment, cable terminations, and cross-connects. The closet is the recognized cross-connect between the backbone cable and horizontal cabling.

*Tight Buffer.* A cable construction where each fiber is tightly buffered by a protective thermoplastic coating to a diameter of 900  $\mu\text{m}$ .

*Transmitter.* An electronic package which converts an electrical signal to an optical signal.

*Wavelength.* The distance between the same two points on adjacent waves; the time required for a wave to complete a single cycle.

*Work Area.* A building space where the occupants interact with telecommunications terminal equipment; i.e. PCs, telephones, and other office equipment.

**Appendix D - Micro OWL Specifications**

Detector Type:-----	Ge (2mm)
Calibrated Wavelengths:-----	850, 1300/1310, 1550
Measurement Range:-----	+5 to -70 dBm (+ versions) +25 to -50 dBm (C+ versions)
Accuracy:-----	±0.15 dB
Resolution:-----	0.01
Battery Life:-----	up to 200 hours (9V)
Connector Type:-----	Universal 2.5mm
Operating Temperature:-----	-10 to 55 C
Storage Temperature:-----	-30 to 70 C
Size:-----	3.48"W x 6.48"H x 1.1"D
Weight:-----	373g (12 oz.)
Data Storage Points:-----	up to 1000
Download Data Points:-----	OWL Reporter Software
Absolute/Relative Measurements:-----	Yes
Battery Capacity Display:-----	Yes
Backlight:-----	Yes
NIST Traceable:-----	Yes

**Appendix E - Warranty Information**

Your Micro OWL comes standard with a one-year limited warranty which covers the meter against manufacturing and assembly defects. Any returns not related to these types of defects are not covered under the warranty. Call tech support at (262) 473-0643 with any warranty concerns you may have.

Over time, the meter may lose its accuracy. This is natural for equipment of this type due to the electronic components used. Re-calibration may be necessary to restore the meter to its original accuracy. Re-calibration is not covered under warranty, but is offered as a service. Call OWL at (262) 473-0643 for more details on our re-calibrations services.

## Appendix F - Cleaning and Care Instructions

The Micro OWL is a sensitive piece of scientific equipment. Great care should be taken when handling and cleaning it.

### **HANDLING TIPS**

- 1) Do NOT drop any piece of scientific equipment, e.g. the Micro OWL. Damage may occur to the case or electronic components on the circuit board may become dislodged, and inaccuracy may occur.
- 2) Keep the meter in its neoprene case when not in use. This will help protect the meter from the elements and accidental droppage.
- 3) Store the meter in a cool dry area when not in use in order to keep the meter in top working condition.
- 4) We recommend not removing the universal connector as it is not necessary for cleaning. Its parts are very fragile, small, and easy to lose.
- 5) Always remember to replace the rubber cap on the connector. This will keep dust and dirt out of it when you are not using the meter.

### **CLEANING TIPS**

- 1) Use only 99% or better Isopropyl alcohol when cleaning the detector. Any less than 99% contains too much water and will begin to corrode the components. 99% Isopropyl alcohol is very flammable, so additional care must be taken when cleaning the detector. 99% Isopropyl alcohol can be purchased at your local drug store.
- 2) Whenever possible, use specially designed 2.5mm cleaning sticks to clean the detector. These do not require alcohol and do not damage the insides of the connector. Do not use sticks or swabs of any other type because they may damage the zirconium ferrule or the coating of the detector inside the connector, or may leave behind dust or fibers that will add loss to the fiber reading.
- 3) The detector port should be cleaned at the beginning and end of the testing day to keep connector loss during testing at a minimum.
- 4) When cleaning the meter itself, do not use any household cleaner that contains ammonia as this will damage any plastic it comes in contact with.
- 5) The case is splash-proof, so it is not necessary to clean the inside of the meter.
- 6) Only use lint-free cloths. Anything else may scratch the plastic of the display.

## Appendix G - Supplies

**MULTI-MODE LIGHT SOURCES**

Dual OWL Dual Wavelength ST Multi-mode Light Source  
850 OWL 850nm ST Multi-mode Light Source  
1300 OWL 1300nm ST Multi-mode Light Source

**SKU #**

DO-1  
DO-850  
DO-1300

**SINGLE MODE LIGHT SOURCES**

Laser OWL Dual Wavelength ST Single Mode Laser Light Source  
Laser OWL Dual Wavelength SC Single Mode Laser Light Source  
Laser OWL Dual Wavelength FC Single Mode Laser Light Source

LO-1ST  
LO-1SC  
LO-1FC

1310 OWL 1310nm ST Single Mode Laser Light Source  
1310 OWL 1310nm SC Single Mode Laser Light Source  
1310 OWL 1310nm FC Single Mode Laser Light Source

LO-1310ST  
LO-1310SC  
LO-1310FC

1550 OWL 1550nm ST Single Mode Laser Light Source  
1550 OWL 1550nm SC Single Mode Laser Light Source  
1550 OWL 1550nm FC Single Mode Laser Light Source

LO-1550ST  
LO-1550SC  
LO-1550FC

## Appendix H - Link Budget Calculation Worksheet

Operating Wavelength

Fiber Type

### Passive Cable System Attenuation

Fiber Loss at Operating Wavelength (Distance x Fiber Loss)

Total Cable Distance  km

Individual Fiber Loss (at operating wavelength)  dB/km

Total Fiber Loss  dB

Connector Loss (Connector Loss x Connector Pairs)

Individual Connector Loss  dB

Number of Connector Pairs

Total Connector Loss  dB

Splice Loss (Splice Loss x Splices)

Individual Splice Loss  dB

Number of Splices

Total Splice Loss  dB

Other Components  dB

Total System Attenuation  dB

(Fiber Loss + Connector Loss + Splice Loss + Other Components)

### Calculate Link Loss Budget

Determine System Gain (Avg. Transmitter Power - Receiver Sensitivity)

Avg. Transmitter Power  dBm

Receiver Sensitivity  dBm @  $10^{-9}$  BER

System Gain  dB

Power Penalties (Operating Margin + Receiver Power Penalties + Repair Margin # Splices at 0.3dB each)

Operating Margin  dB

Receiver Power Penalties  dB

Repair Margin  dB

Total Power Penalty  dB

Determine link Loss Budget (System Gain - Power Penalty)

System Gain  dB

Total Power Penalty  dB

Total Link Loss Budget  dB

### Verify Performance

Verify Adequate Power (Total Link Loss Budget - Total System Attenuation)

Total Link Loss Budget  dB

Total System Attenuation  dB

System Performance Margin\*  dB

\* System Performance Margin must be greater than 0 dB in order for the system to operate using the specified electronics.

## Appendix I - Reference jumper setup

Your test jumpers must be cleaned and inspected prior to using them for fiber link testing. You should have one jumper for the power meter side of the test, and one jumper for each of the connector ports on your light source. Make sure that these patch cords match the fiber under test (i.e. same fiber type, same core/cladding size, same connector type).

Use the following steps to set up your reference jumpers for link testing:

Step 1 - Connect the first jumper to the power meter and light source. Verify that it is working properly and not introducing significant loss to the test. Disconnect this patch cord from the light source and meter and set it aside.

Step 2 - Connect the other patch cord(s) to the light source. If you have a dual wavelength light source with two connector ports, then you will need to connect one jumper to each port.

Step 3 - MULTI-MODE ONLY. If you are testing multi-mode fibers, you will need to wrap each of the jumpers connected to the light source around a ½" mandrel at least 5 times. This is done to achieve Equilibrium Mode Distribution (EMD), which eliminates unwanted optical energy that can cause inaccurate test results.

Step 4 - Run the Link Wizard. You will be prompted to connect the patch cords during this process, once for each wavelength. See Unit 3 for detailed instructions.

NOTE: Do NOT remove the patch cords from the light source until you have completed testing all of the fibers in the link. Disconnecting the test jumper from the light source and re-connecting it will cause the Link Wizard reference to be incorrect, thereby producing incorrect readings, and may cause a link to fail.



Multi-mode  
Reference



Single Mode  
Reference